

★ DO NOT DISCARD CAREFULLY THIS INSTRUCTION MANUAL UNTIL ALL THE TUBES IN THIS BOX ARE USED UP.

1. PERFORMANCE:

Measuring Range	: 0.5 - 10 ppm
and Sampling Time	: 2.5 minutes
Colour Change:	: White → Pale Brown
Detectable Limit:	: 0.1 ppm
Operating temperature:	: 5 - 40 °C (41-104°F)

⚠ CAUTION

1. THE DETECTOR TUBE CONTAINS CHEMICAL REAGENTS.
2. DO NOT TOUCH THESE REAGENTS DIRECTLY ONCE TUBES WERE BROKEN.
3. KEEP THE TUBES OUT OF THE REACH OF CHILDREN.

NOTICE

1. DO NOT USE THIS TUBE OUTSIDE THE STATED OPERATING TEMPERATURE RANGE.
2. STORE TUBES IN A COOL AND DARK PLACE (0-25 °C/32-77°F), AND USE BEFORE EXPIRATION DATE PRINTED ON THE TOP OF THE BOX.
3. PRIOR TO USE, READ ITEM 7 "USER RESPONSIBILITY" CAREFULLY.
4. READ THE CONCENTRATION IMMEDIATELY AFTER DRAWING THE SAMPLE.

2. SAMPLING AND MEASUREMENT:

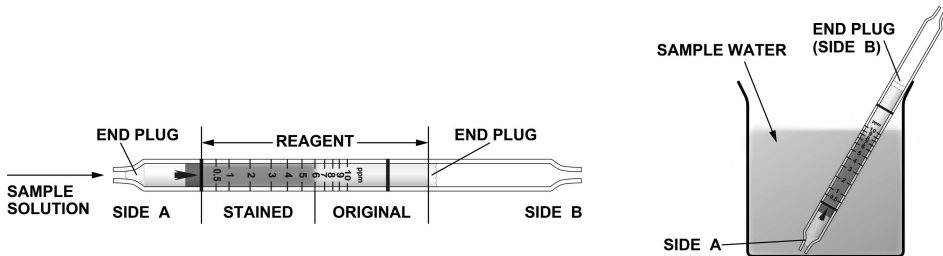


Fig.1

- ① Break both ends of the detector tube.

⚠ CAUTION SAFETY GLASSES AND GLOVES SHOULD BE WORN TO PREVENT INJURY FROM SPLINTERING GLASS.

- ② Immerse the end of the tube with side A (Arrow mark) into the prepared sample solution. Capillary action occurs immediately and the sample rises through the reagent. Sulphide ion in the sample makes a pale brown stain.
- ③ When the sample rises up to the top end plug (side B), remove the tube from the sample.
- ④ On completion of sampling, read the scale at the maximum point of the stained layer.
- ⑤ In case that concentration of sample solution is supposed to be above 10ppm (full scale) dilute the sample solution accurately with distilled water. Then measure the sample solution and multiply its reading by dilution ratio. You can get real concentration in the way of above mentioned procedure.

SPECIAL NOTE: When the top of the stained layer is unclear, read the scale at the centre between the longest and shortest points.

3. CORRECTION FOR AMBIENT CONDITIONS:

Temperature; No temperature correction is necessary at the temperature of 5 °C (41°F) to 40 °C (104°F).


4. INTERFERENCE:

Coexistence of more than 1000ppm of Carbonate ion will give lower reading.

Coexistence of more than 2000ppm of Chloride ion will give higher reading.

PH value within 7-14 does not affect the reading value.

5. CHEMICAL REACTION IN THE DETECTOR TUBE:



6. DISPOSAL OF TUBES:

USED TUBES SHOULD BE DISPOSED CAREFULLY ACCORDING TO RELEVANT REGULATIONS, IF ANY.

7. USER RESPONSIBILITY:

It is the sole responsibility of the user of to ensure that detector tubes are not used beyond their expiration date or have a colour change different to that stated in the Performance specifications. The Manufacturer and Manufacturer's Distributor shall not be otherwise liable for any incorrect measurement or any damages, whether damages result from negligence or otherwise.

※ Product specifications are subject to change without any prior notice.

IME2001/1

Printed in Japan