



INSTRUCTION MANUAL METHYL ETHYL KETONE DETECTOR TUBE

No.139SD

(ISOBUTYL ACETATE, ISOPROPYL ACETATE, BUTYL ACETATE, PROPYL ACETATE, 1,4-DIOXANE WITH CONVERSION CHART)

- ★ READ CAREFULLY THIS INSTRUCTION MANUAL AND THE INSTRUCTIONS OF THE ASPIRATING PUMP PRIOR TO USING THIS PRODUCT.
- ★ DO NOT DISCARD THIS INSTRUCTION MANUAL UNTIL ALL THE TUBES IN THIS BOX ARE USED UP.

1. PERFORMANCE:

Measuring Range	: 0.01 - 1.4 %
and Pump Stroke	: 2 pump strokes
Sampling Time	: 3 minutes
Colour Change	: Orange → Brownish green
Detectable Limit	: 10 ppm
Operating Temperature	: 0 - 40 °C (32 - 104°F) (No correction is necessary.)
Aspirating Pump	: Model AP-20, AP-20S, 400B, AP-1, AP-1S or 400A

※ By using conversion charts undermentioned (REFER TO ITEM 4. CONVERSION CHART), following gases can be detected.

Gases to Measured	Measuring Range	Number of pump strokes	Operating Temperature
Isobutyl acetate	0.01 - 1.4 %	2 (200mL)	*0 - 40 °C (32-104°F)
Isopropyl acetate	0.01 - 1.2 %	2 (200mL)	*0 - 40 °C (32-104°F)
Butyl acetate	0.01 - 1.0 %	2 (200mL)	*0 - 40 °C (32-104°F)
Propyl acetate	0.01 - 1.4 %	2 (200mL)	*0 - 40 °C (32-104°F)
1,4-Dioxane	0.05 - 2.5 %	2 (200mL)	*0 - 40 °C (32-104°F)

*No temperature correction is necessary.

CAUTION

1. THE DETECTOR TUBE CONTAINS CHEMICAL REAGENTS.
2. DO NOT TOUCH THESE REAGENTS DIRECTLY ONCE TUBES WERE BROKEN.
3. KEEP THE TUBES OUT OF THE REACH OF CHILDREN.

NOTICE

1. USE ONLY WITH PUMP MODELS AP-20, AP-20S, 400B, AP-1, AP-1S OR 400A. OTHERWISE, CONSIDERABLE ERROR IN INDICATION MAY OCCUR.
2. BEFORE TESTING, CHECK THE ASPIRATING PUMP FOR LEAKS (REFER TO ITEM 9. INSPECTION OF ASPIRATING PUMP). ANY PUMPS SHOWING SIGNS OF LEAKAGE SHOULD BE CORRECTED BEFORE USE.
3. DO NOT USE THIS TUBE OUTSIDE THE STATED OPERATING TEMPERATURE RANGE.
4. STORE TUBES IN A COOL AND THE DARK PLACE (0-25 °C/32-77°F), AND USE BEFORE EXPIRATION DATE PRINTED ON THE TOP OF THE BOX.
5. PRIOR TO USE, READ CAREFULLY ITEM 10. USER RESPONSIBILITY.
6. READ THE CONCENTRATION IMMEDIATELY AFTER MEASUREMENT.

2. SAMPLING AND MEASUREMENT:

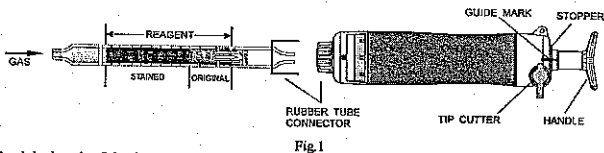


Fig.1

- ① Break both ends of the detector tube.

CAUTION SAFETY GLASSES AND GLOVES SHOULD BE WORN TO PREVENT INJURY FROM SPLINTERING GLASS.

- ② Insert the detector tube into the aspirating pump securely as shown in Fig.1. (Arrow mark shall point to the pump.)
- ③ Align the guide marks on the shaft and stopper of the aspirating pump.
- ④ Pull the pump handle at a full stroke until it locks and wait for 1.5 minutes or until the completion of sampling is confirmed with the flow indicator of the pump (See descriptions about the flow indicator in the instruction manual of the pump).
- ⑤ Push back the handle without removing the detector tube from the rubber tube connector so that air in the pump will be discharged perfectly. Then repeat the step ③~④ once more.
- ⑥ On completion of sampling, read the scale at the maximum point of the stained layer.

- SPECIAL NOTE:**
- I. The scale is calibrated at 20 °C (68°F), 50%RH, and 1013hPa. Readings obtained in other circumstances should be corrected (REFER TO ITEM 3. CORRECTION FOR AMBIENT CONDITIONS).
 - II. When the maximum point of the stained layer is unclear or oblique, read the scale at the centre between the longest and shortest points.


3. CORRECTION FOR AMBIENT CONDITIONS:

- ① Temperature, No correction is necessary.
- ② Humidity, No corrections is necessary.
- ③ Atmospheric Pressure,


$$\text{True concentration} = \text{Tube reading} \times \frac{1013}{\text{Atmospheric pressure (in hPa)}}$$

4. CONVERSION CHART


ISOBUTYL ACETATE




ISOPROPYL ACETATE




BUTYL ACETATE



PROPYL ACETATE



1,4-DIOXANE



5. INTERFERENCES:

Coexistence of more than 3% of Acetylene or 0.2% of Propane changes the colour of whole reagent to brown stains and give higher readings. More than 50ppm of the other organic gases or vapors except Halogenated hydrocarbons produce a similar stains and give higher readings.

6. CHEMICAL REACTION IN THE DETECTOR TUBE:

Methyl ethyl ketone	CH ₃ COCH ₂ CH ₃	+ C ⁶⁺ + H ₂ SO ₄	→ C ⁶⁺
Isobutyl acetate	CH ₃ COCH ₂ CH(CH ₃) ₂	+ C ⁶⁺ + H ₂ SO ₄	→ C ⁶⁺
Isopropyl acetate	CH ₃ COCH(CH ₃) ₂	+ C ⁶⁺ + H ₂ SO ₄	→ C ⁶⁺
Butyl acetate	CH ₃ CO ₂ C ₄ H ₉	+ C ⁶⁺ + H ₂ SO ₄	→ C ⁶⁺
Propyl acetate	CH ₃ CO ₂ C ₃ H ₇	+ C ⁶⁺ + H ₂ SO ₄	→ C ⁶⁺
1,4-Dioxane	C ₄ H ₈ O ₂	+ C ⁶⁺ + H ₂ SO ₄	→ C ⁶⁺

7. DISPOSAL OF TUBES:

USED TUBES SHOULD BE DISPOSED CAREFULLY ACCORDING TO RELEVANT REGULATIONS, IF ANY.

8. HAZARDOUS AND DANGEROUS PROPERTIES OF :

Methyl ethyl ketone	TLV-TWA ◆: 200 ppm	Explosion range in air:	1.7 - 11.5 %
Isobutyl acetate	TLV-TWA ◆: 150 ppm	Explosion range in air:	1.3 - 10.5 %
Isopropyl acetate	TLV-TWA ◆: 100 ppm	Explosion range in air:	1.8 - 7.8 %
Butyl acetate	TLV-TWA ◆: 150 ppm	Explosion range in air:	1.2 - 7.6 %
Propyl acetate	TLV-TWA ◆: 200 ppm	Explosion range in air:	1.7 - 8.0 %
1,4-Dioxane	TLV-TWA ◆: 20 ppm	Explosion range in air:	2.0 - 22.0 %

◆ Threshold Limit Value established by the American Conference of Governmental Industrial Hygienists, 2008.

9. INSPECTION OF ASPIRATING PUMP:

Checking for leaks;

- ① Insert a sealed, unbroken detector tube into the pump.
- ② Align the guide marks on the shaft and stopper of the pump.
- ③ Pull the handle to a full stroke and wait for 1 minute.
- ④ Unhook the handle and allow it to return slowly into the pump by holding the cylinder and handle securely. **CAUTION HANDLE WILL TEND TO SNAP BACK INTO THE PUMP QUICKLY.**
- ⑤ If the handle returns completely to the original position, the performance is satisfactory. Otherwise, refer to maintenance procedures shown in the instruction manual of the pump to correct the leakage.

10. USER RESPONSIBILITY:

It is the sole responsibility of the user of this equipment to ensure that the equipment is operated, maintained, and repaired in strict accordance with these instructions and the instructions provided with each Model AP-20, AP-20S, 400B, AP-1, AP-1S or 400A aspirating pump, and that detector tubes are not used which are either beyond their expiration date or have a colour change different to that stated in the Performance specifications. The Manufacturer and Manufacturer's Distributors shall not be otherwise liable for any incorrect measurement or any damages, whether damages result from negligence or otherwise.

Printed in Japan

IME1391